


SEATING TISSUE LOAD MANAGEMENT ALGORITHM



Note: This algorithm is meant as a guide, and is not a substitute for clinical judgment. Regardless of product selection, a full assessment of skin status and repositioning is required according to best clinical practice.

Seat/Back Combination Products for Prevention with Positioning
LOW to MODERATE risk

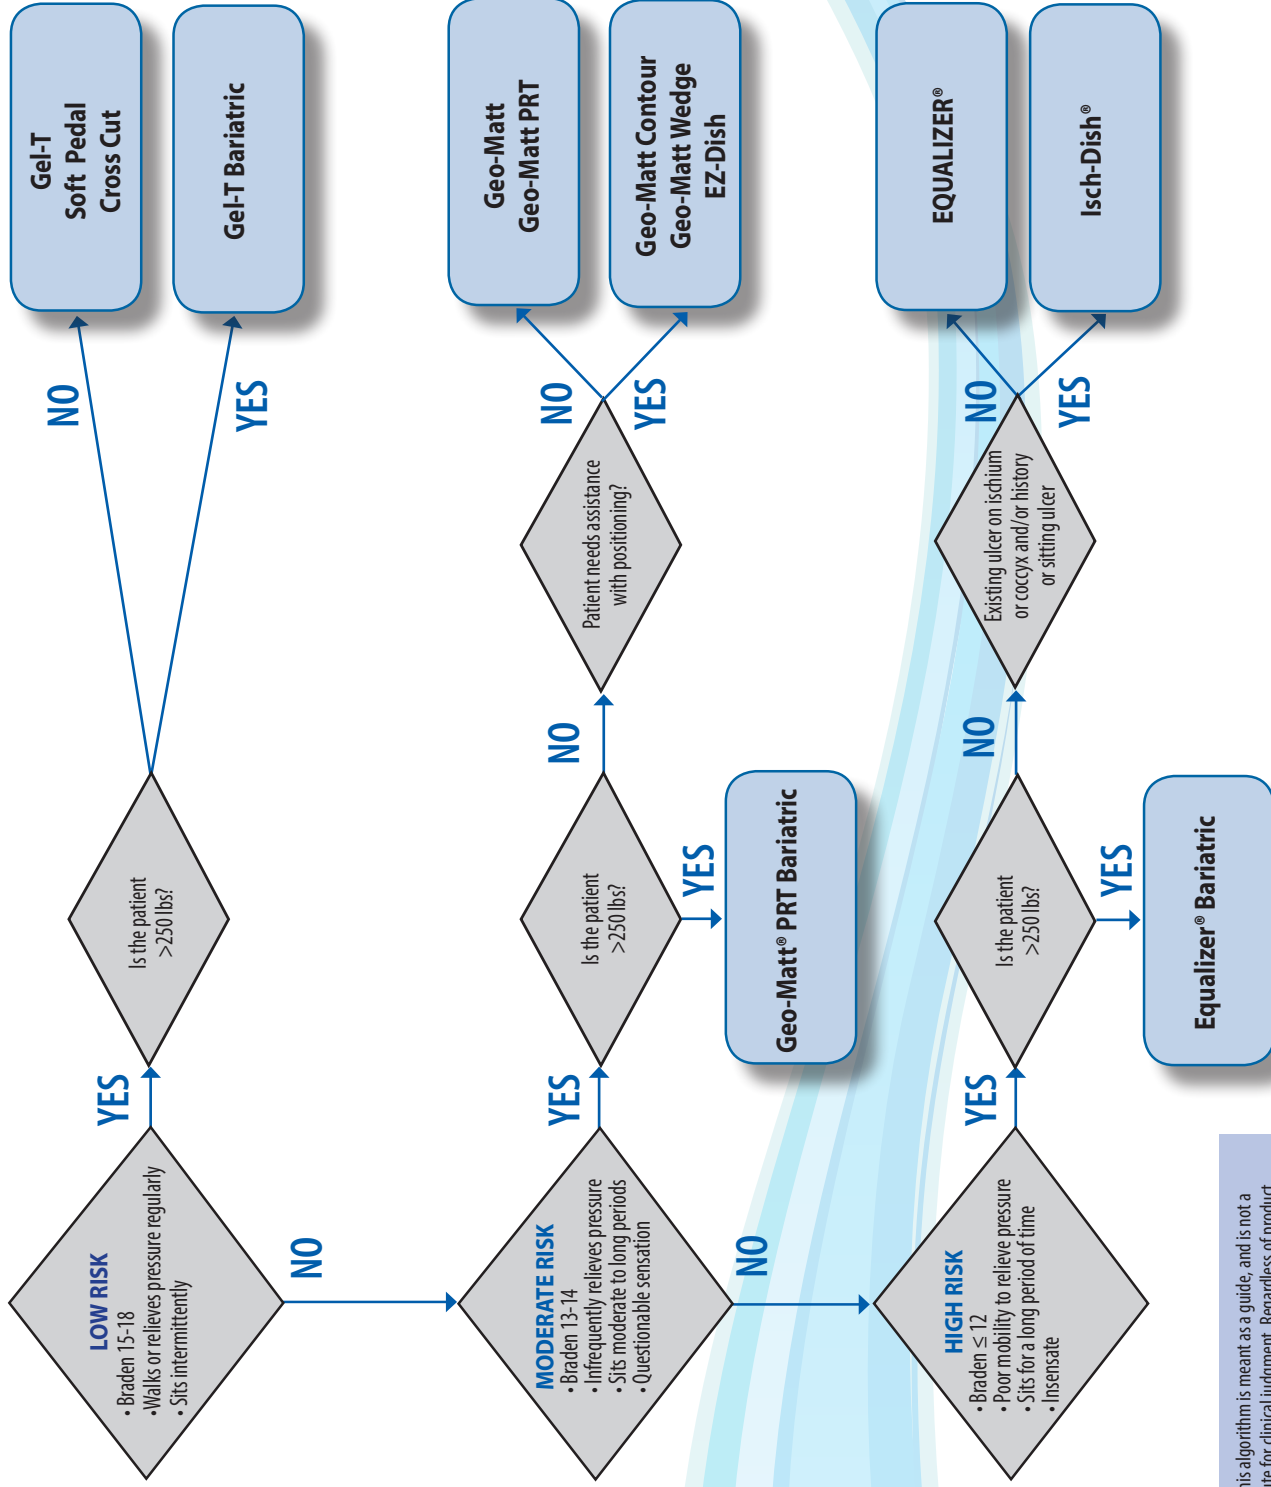


Short Wave®
Seat and Back Cushion

Geo-Wave®
Specialty Chair Cushion